

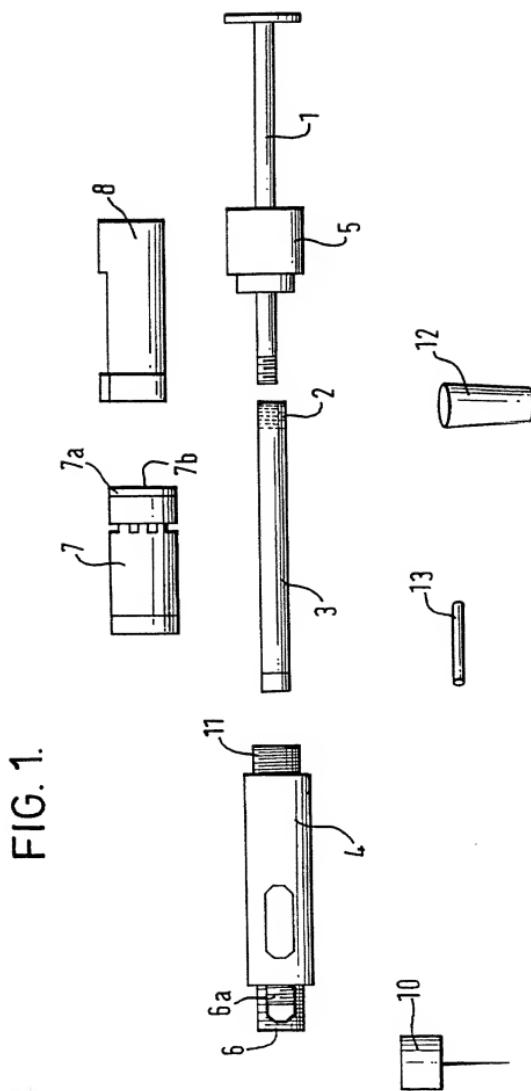


1 / 17

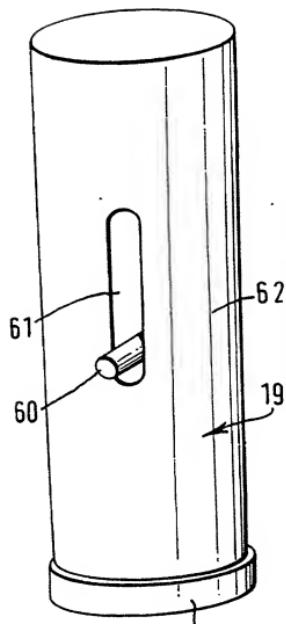

SUBSTITUTE SHEET (RULE 26)

10013080-121001

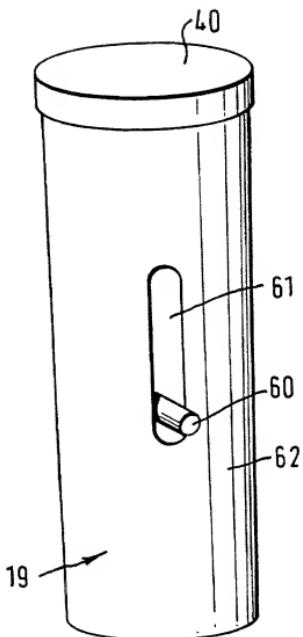

TRIDAT® OSMOTEST

FIG. 3a.

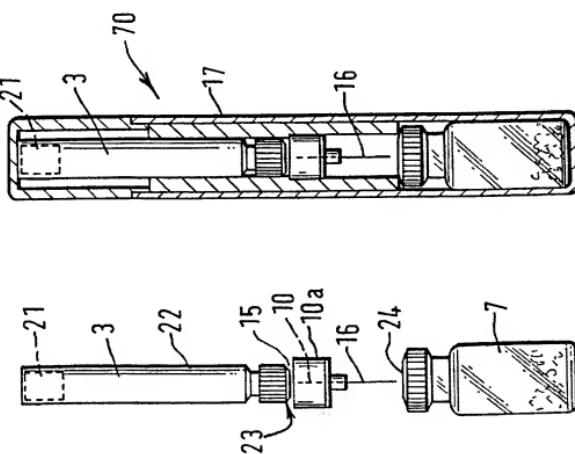


FIG. 3b.

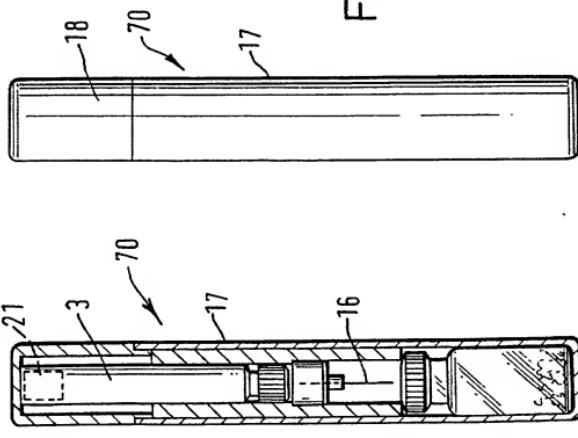


FIG. 3c.

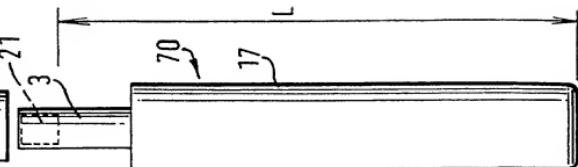
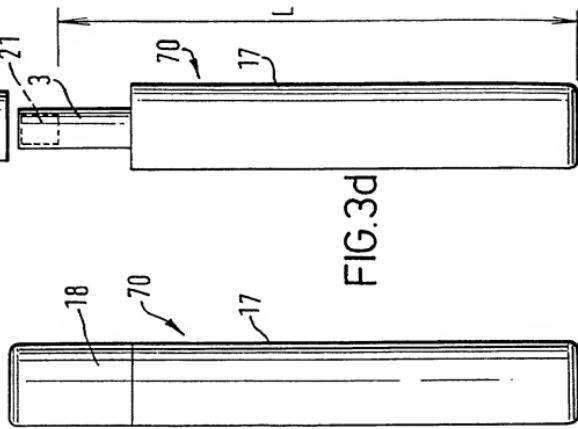


FIG. 3d

4 / 17

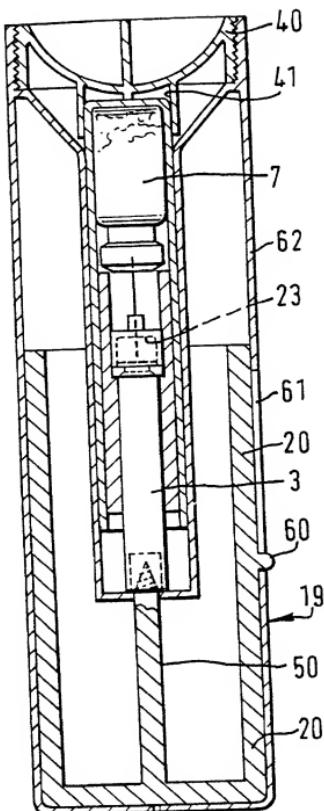


FIG. 4a.

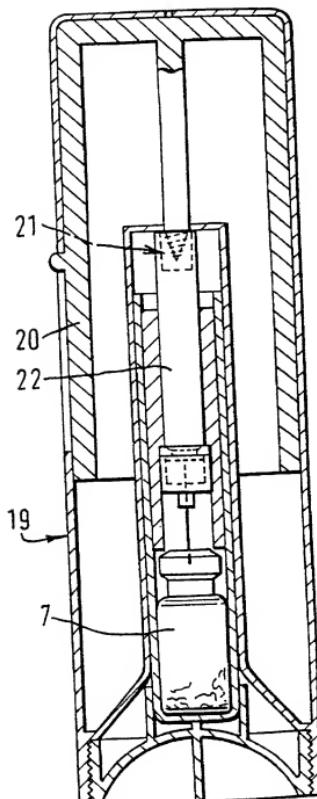


FIG. 4b.

5 / 17

10013080.121001

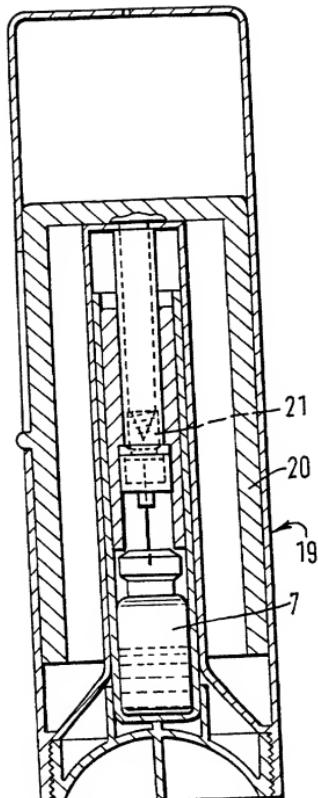


FIG. 4c.

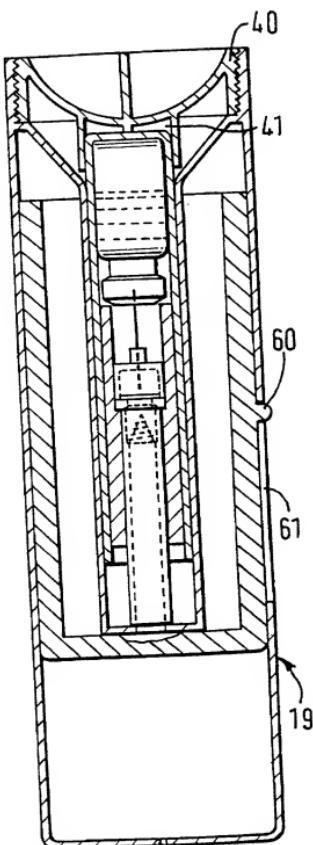


FIG. 4d.

6 / 17



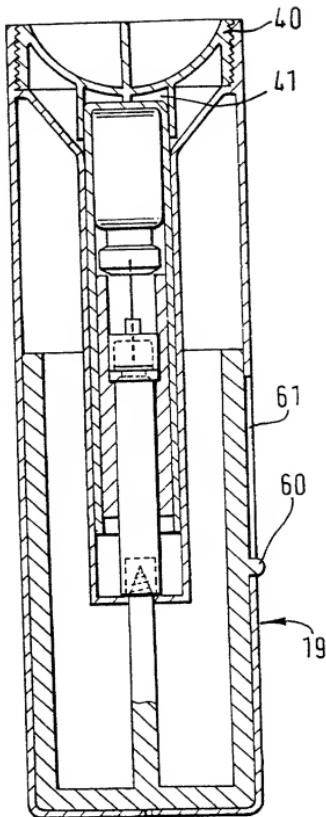


FIG. 4e.

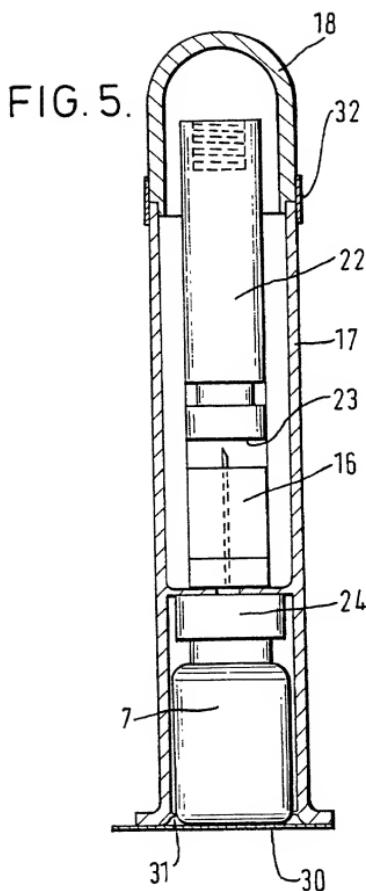

8 / 17

FIG. 6a.

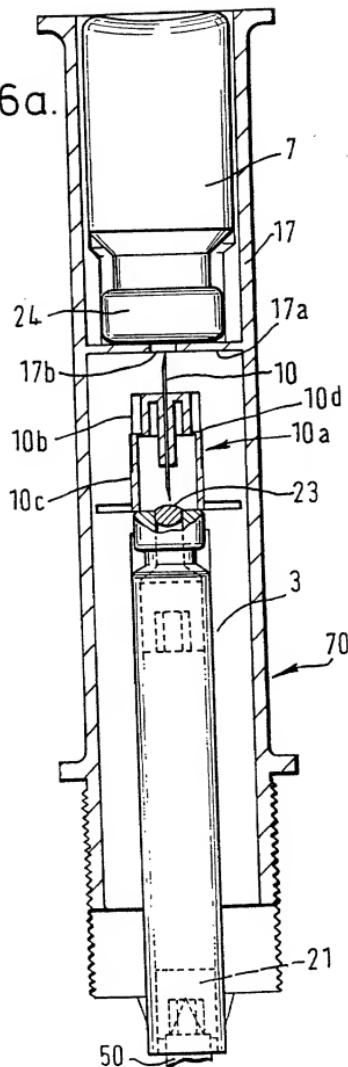


SUBSTITUTE SHEET (RULE 26)

10013080-121001


9 / 17

FIG. 6b.

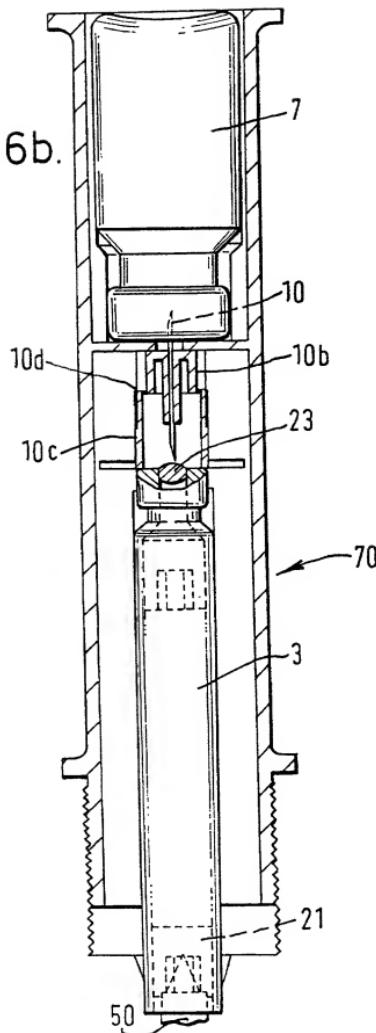


10 / 17

FIG. 6c.

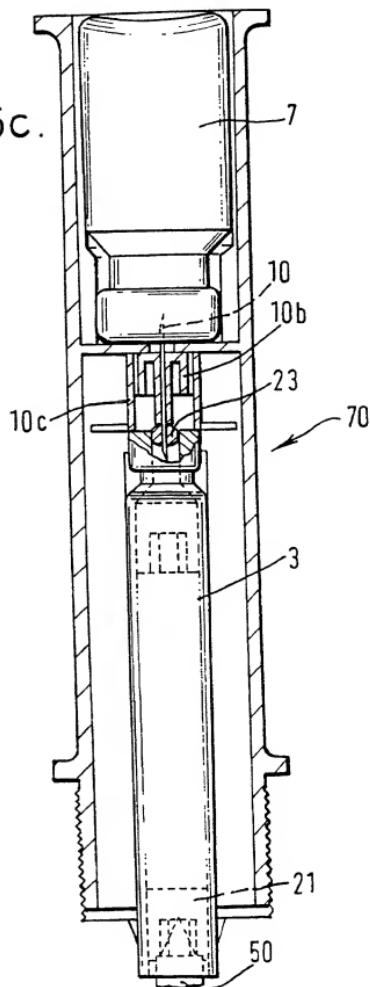


11 / 17

FIG. 7.

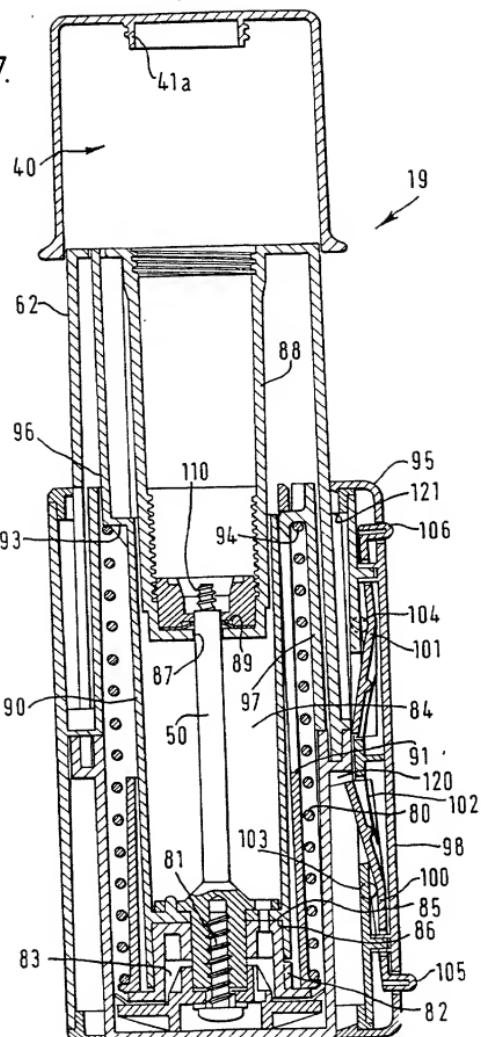


12 / 17

FIG. 8.

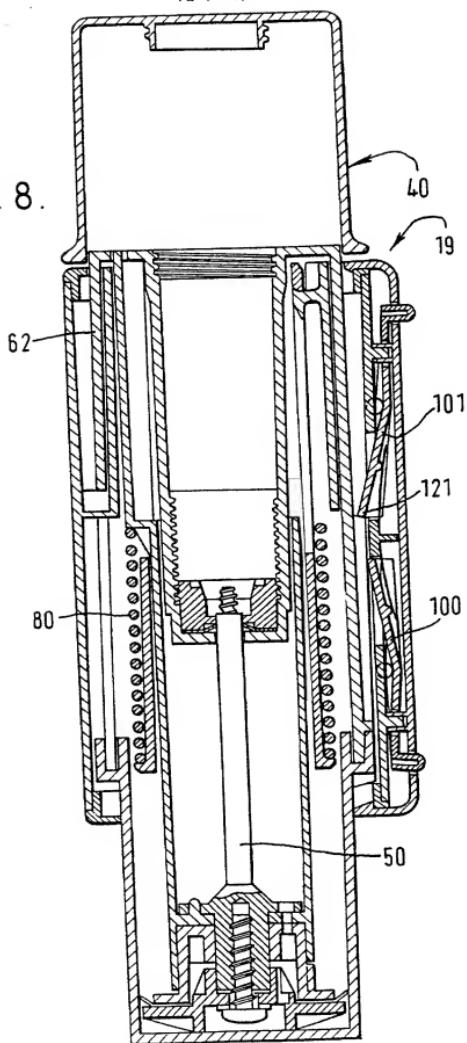


13 / 17

FIG. 9.

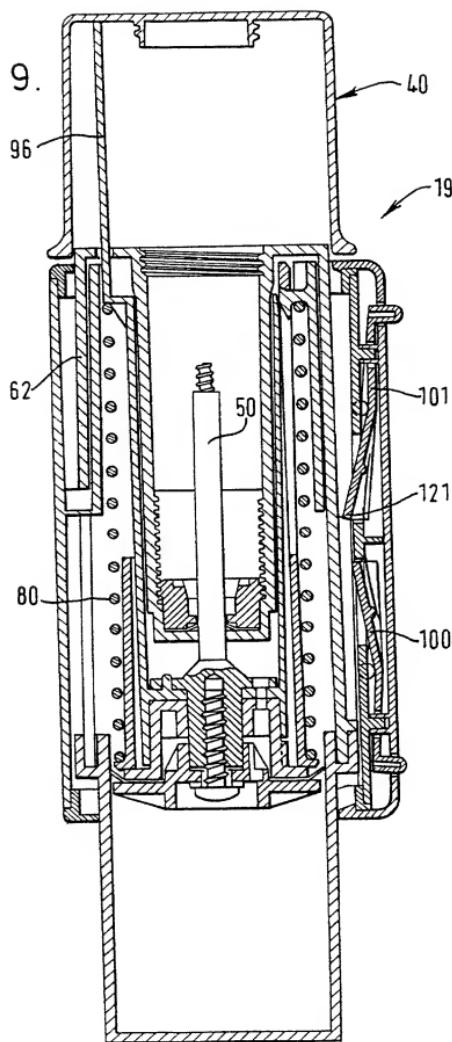


14 / 17

FIG. 10.

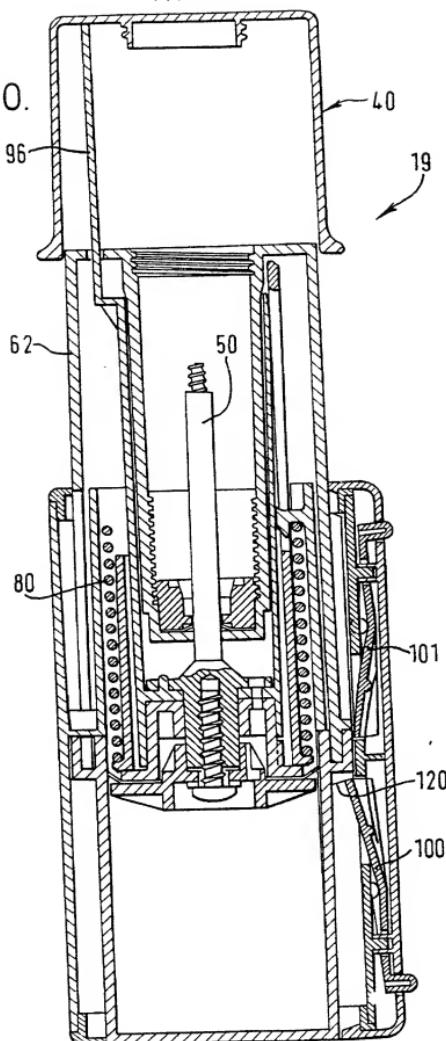


15 / 17

FIG.11i.



106 FIG.11g.



105 FIG.11e.



FIG.11a.
105
106

FIG.11i.




FIG.11h.




105 FIG.11f.

FIG.11d.

105 FIG.11b.


FIG.11h.

16 / 17

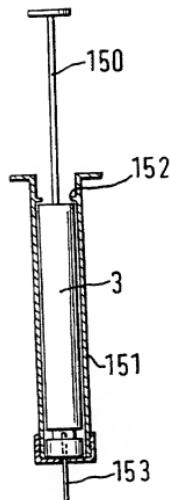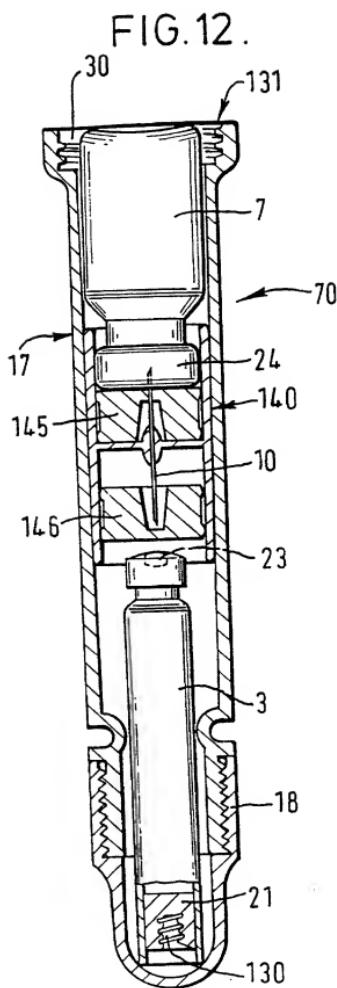

17 / 17

FIG.13.

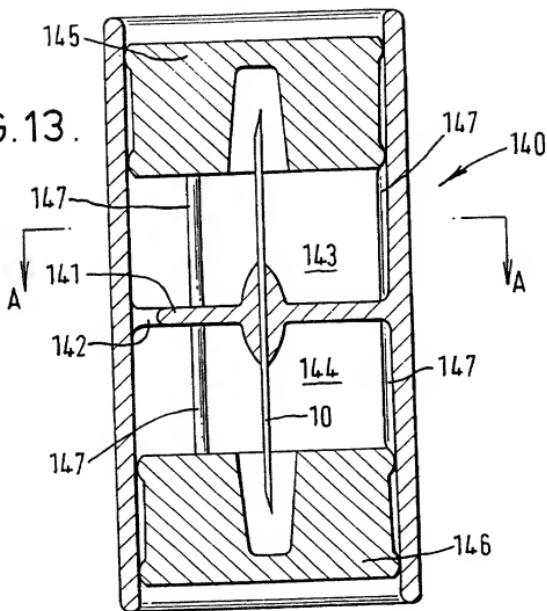

100013080-121001

FIG.14.

